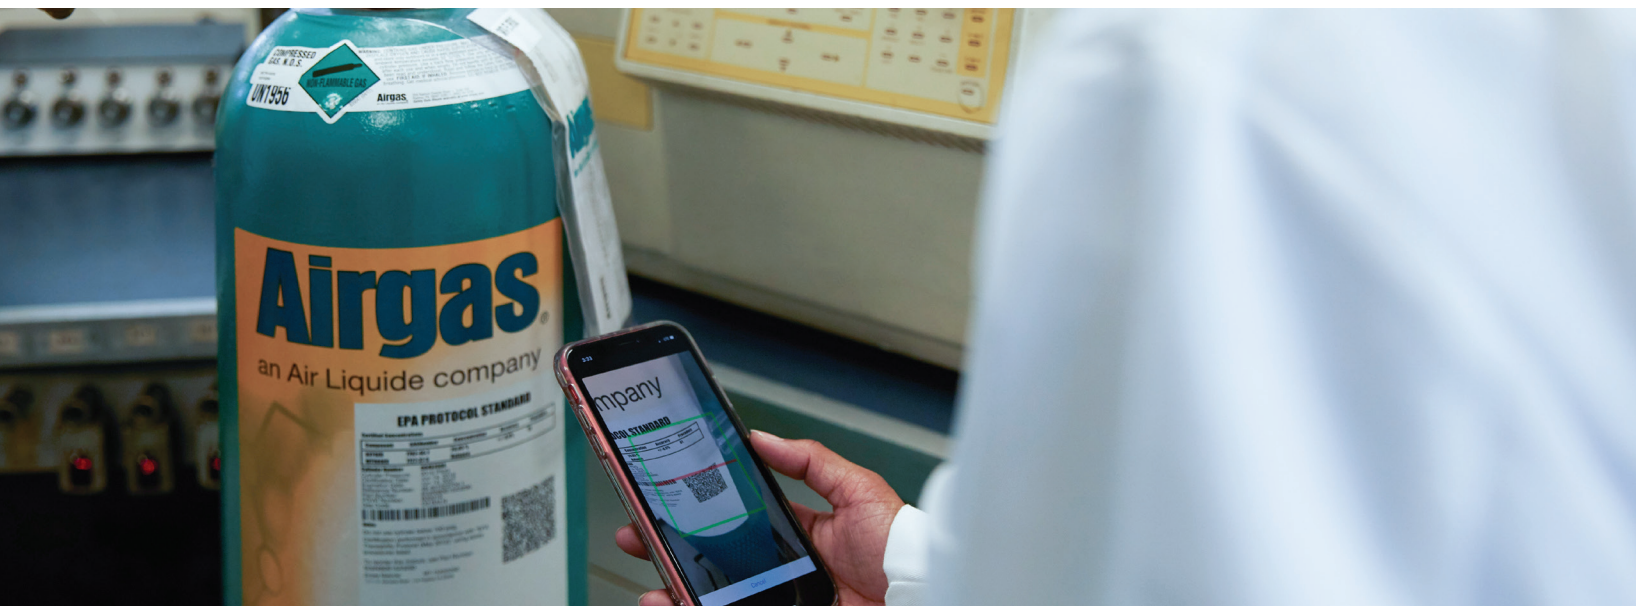# Airgas

an Air Liquide company

Airgas SRVS App

Streamline gas data management

- Save time and simplify management of your Certificates of Analysis
- Reduce errors in records keeping
- Ensure regulatory compliance

Scan. Record. View. Send.
Automatic export reduces risk

Eliminate manual data entry and associated errors, and quickly move important data from your Certificate of Analysis to your reporting system electronically using the Airgas SRVS app. Powered by our patented and proprietary technology that includes new features designed for efficiency, simply scan the QR code or cylinder barcode to view and send this information directly into your data management software. Now get peace of mind with error-free data intended to support your regulatory compliance.

Airgas.com

Streamline gas data management
Eliminate mistakes, save time, ensure regulatory compliance

Are you ready to improve your gas analysis data transfer from your cylinder's Certificate of Analysis into your data management software? The Airgas SRVS app with new and improved features quickly scans the QR code on your certificate or cylinder barcode to capture relevant and important cylinder information and upload it — no need to re-key cylinder data into various reporting systems, databases or profiles.

- Continuously scan embedded data via QR or bar codes without interruption - vibration indicates when scan is complete
- View data and email in CSV/Excel, RTF/Word or PDF file formats
- Easily transfer information by selecting your send-to location: DAS provider interfaces, email, text, cloud drive (including Google, Dropbox, etc.) and other mobile apps
- Improve cylinder management by specifying the exact locations of your cylinders
- Maintain control of your data and file security
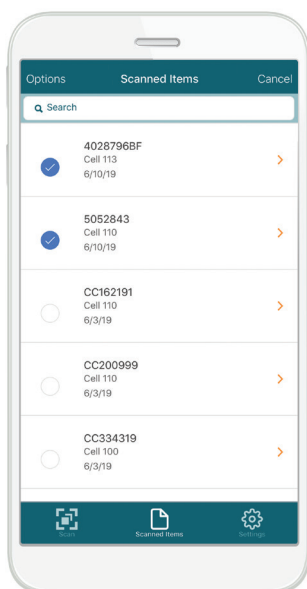- Convenient built-in flashlight

Managing your Certificates of Analysis and critical gas data is easier now – download the Airgas SRVS app now from the App Store or Google Play
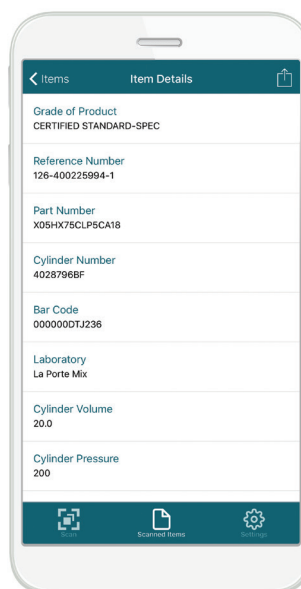
Scan

Airgas.
an Air Liquide company

TAP TO SCAN

Scan | Scanned Items | Settings

Record

Options | Scanned Items | Cancel

Search

4028796BF
Cell 113
6/10/19

5052843
Cell 110
6/10/19

CC162191
Cell 110
6/3/19

CC200999
Cell 110
6/3/19

CC334319
Cell 100
6/3/19

Scan | Scanned Items | Settings

View

Items | Item Details

Grade of Product
CERTIFIED STANDARD-SPEC

Reference Number
126-400225994-1

Part Number
X05HX75CLP5CA18

Cylinder Number
4028796BF

Bar Code
000000DTJ236

Laboratory
La Porte Mix

Cylinder Volume
20.0

Cylinder Pressure
200

Scan | Scanned Items | Settings

Send

Items | Item Details

Grade of Product
CERTIFIED STANDARD-SPEC

Reference Number
126-400225994-1

Part Number
X05HX75CLP5CA18

AirDrop. Share instantly with people nearby. If they turn on AirDrop from Control Center on iOS or from Finder on the Mac, you'll see their names here. Just tap to share.

Message | Gmail | Drive | OneDrive | Add to Notes

Copy | Save to Files | More

Cancel

Contact us
866.924.7427 | EPA.Protocols@airgas.com

MCM-408 | ©2019 Airgas, Inc. | Printed in the U.S.A.

Airgas.
an Air Liquide company